



ES

WKB003  
Manual de instrucciones  
WE-2020-WKB003-1

# RADIOFRECUENCIA MONOPOLAR

## ADVERTENCIA

• Nunca, en ninguna circunstancia, intente abrir o inspeccionar los componentes o accesorios internos de la máquina. Si fuera necesaria una inspección, por favor póngase en contacto con su proveedor o un técnico debidamente cualificado.

• No utilice nunca la unidad en ambientes húmedos o insuficientemente ventilados, como zonas de aguas, baños, etc., con el fin de prevenir daños en los componentes eléctricos de su equipo.

• Nunca utilice el equipo al aire libre, las inclemencias meteorológicas pueden causar daños.

• Si el cable eléctrico estuviera roto, solicite a un profesional que le suministre otro y lo cambie para evitar riesgos, o contacte con el proveedor.

## DECLARACIÓN DE CONFORMIDAD CE

Este producto cumple lo estipulado en las siguientes directivas:

1. Las medidas de la Directiva sobre Baja Tensión: 2014/35/EU

2. Las medidas de la Directiva de Compatibilidad Electromagnética: 2014/30/EU

## RECICLAJE



Cuando aparezca este símbolo en cualquiera de nuestros productos eléctricos o su embalaje, esto significa que dichos productos no deben tratarse como residuos domésticos convencionales en Europa. Para asegurar un tratamiento de residuos adecuado, hágalo de acuerdo con las leyes locales o según convenga para el desecho de equipos eléctricos. Esto ayudará a preservar el medio ambiente y mejorar los estándares de protección medioambiental en relación con el tratamiento de residuos eléctricos.

## ¡BIENVENIDO!

Muchas gracias por su compra. Por favor, lea detenidamente las instrucciones antes de utilizar el equipo. También puede pedir orientación a un profesional para asegurarse de que está utilizando el equipo correctamente. No aceptaremos ninguna responsabilidad por los accidentes que ocurran debido a un manejo incorrecto.



La empresa se reserva el derecho de corregir detalles de los equipos, sin previo aviso. Si encuentra algún error en estas instrucciones, por favor no dude en enviarnos un e-mail para informarnos y que podamos corregirlos.

## CONTENIDO DEL PAQUETE

• Estos componentes están sujetos a cambio sin previo aviso.

• El aspecto del producto puede diferir de la imagen.

Nº	PRODUCTO	CANT
1	SONDA CORPORAL	1
2	SONDA FACIAL	1
3	SONDA OJOS	1
4	PLACA RETORNO	1
5	UNIDAD PRINCIPAL	1
6	CABLE CONEXIÓN	1

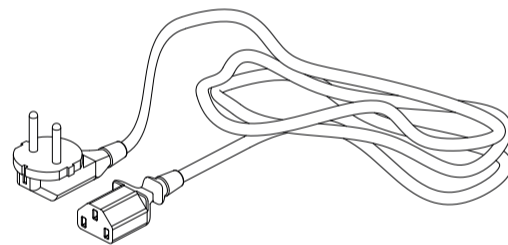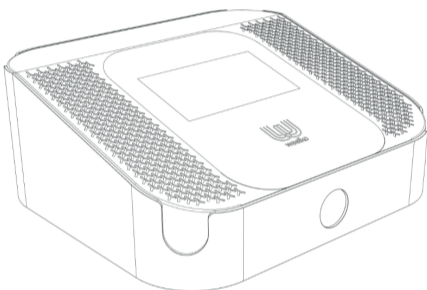

## INSTRUCCIONES DE USO

1. Conecte el cable de alimentación en el panel trasero.

2. Conecte correctamente las sondas y la placa de retorno en el panel trasero.

3. Encienda el botón en el panel frontal y haga clic en el logo Weelko de la pantalla para proceder a seleccionar los menús deseados.

4. Haga clic en el botón "mono.face" si quiere utilizar la sonda facial y la de los ojos y en el botón "mono.body" si quiere utilizar la sonda corporal. La sonda para los ojos se conecta en la misma conexión que la sonda facial, así que para utilizar una de ellas se tiene que desenchufar la otra..

5. Utilice gel específico para radiofrecuencia o glicerina. Aplique una cantidad suficiente en la piel del paciente antes de poner la sonda en contacto con la piel.

6. El menú "LEVEL" permite regular la intensidad en diez niveles.



7. El menú "TIME" permite escoger el tiempo de tratamiento. El programa predeterminado es de 30 minutos.

8. El menú "MODE" permite escoger la onda. El equipo cuenta con tres tipos de 3 onda.

9. Seleccione "PLAY/PAUSE" para empezar o pausar el tratamiento.

## MANTENIMIENTO

• Limpie las sondas con un trapo húmedo después de cada tratamiento.

## PRECAUCIÓN

• Los tratamientos de radiofrecuencia no se deben extender durante un largo periodo de tiempo. La duración recomendada es de 10 minutos para los tratamientos faciales y 20 minutos para los tratamientos corporales. En cualquier caso, no prolongar los tratamientos más allá de 60 minutos.

• Para evitar quemaduras en el paciente, nunca olvide de colocar la placa corporal en contacto con la piel.

• Durante la aplicación del tratamiento, aplicar los electrodos sobre la piel realizando círculos constantemente sin dejar de realizar movimientos en ningún momento. No dejar el electrodo fijado en una zona, se podrían producir quemaduras.

• Compruebe con el paciente que la intensidad es la adecuada a lo largo del tratamiento.

• El paciente y el profesional deben asegurarse de que no llevan objetos metálicos consigo durante el tratamiento.

• Se recomienda al profesional el uso de guantes aislantes durante el tratamiento.

## ACCESORIOS

Nº	PRODUCTO
1	SONDA CORPORAL
2	SONDA FACIAL
3	SONDA OJOS
4	PLACA RETORNO

## FICHA TÉCNICA

Pesos y tamaños	Tamaño embalaje (cm)	51x45x22
	Peso bruto (Kg)	9
	Tamaño consola (cm)	34x38x15
Características eléctricas	Voltaje nominal	220V ~ 240V
	Frecuencia	50Hz/60Hz
	Potencia	150 W



EN

WKB003  
Instruction Manual  
WE-2020-WKB003-1

# MONOPOLAR RADIOFREQUENCY

## WARNING

• Never under any circumstances attempt to open or inspect the internal components or accessories of the machine. If an inspection becomes necessary, please contact your supplier or a suitably competent technician.

• Never use the unit in humid or poorly ventilated environments, such as wet rooms, bathrooms, etc. to prevent damage to the electrical components of your unit.

• Never use the unit outdoors; exposure to the elements can cause damage.

• If the power cord was destroyed, please ask a professional to service and replace it to avoid hazards, or contact the dealer for service.

• Do not use on pregnant women, on people with pace-makers (any electrical or rhythmic heart-regulating device) or with skin infections.


## EC-DECLARATION OF COMPLIANCE

This product meets the following requirements:

1. Conditions set out in the Low Voltage Directive: 2014/35/EU

2. Conditions set out in the Electromagnetic Compatibility Directive: 2014/30/EU

## RECYCLING

 Whenever any of our electrical products or their presentation packaging bear this symbol, it means that these products should not be treated as conventional household waste in Europe. To ensure proper treatment of this waste, dispose of it in accordance with local laws or as required for the disposal of electrical equipment. This initiative will help preserve save natural resources and improve standards of environmental protection in regard to the treatment of electrical waste.

## WELCOME!

Thank you very much for purchase. Please read the instructions carefully before operating the instrument. You can also ask a professional for guidance to make sure you are using the instrument correctly. We will accept no responsibility for any accidents that occur due to



incorrect operation.

The company reserves the right to amend the details of the instruments with no prior notice. If any mistakes are found in these instructions, please feel free to send us an e-mail informing us so that we can correct them.

## PACKAGE CONTENTS


- These components are subject to change without prior notice.
- Appearance of product may differ from the image.

No.	PRODUCT	QTY.
1	BODY ELECTRODES	1
2	FACE ELECTRODES	1
3	EYE ELECTRODES	1
4	NEGATIVE PLATE	1
5	MAIN UNIT	1
6	POWER CORD	1

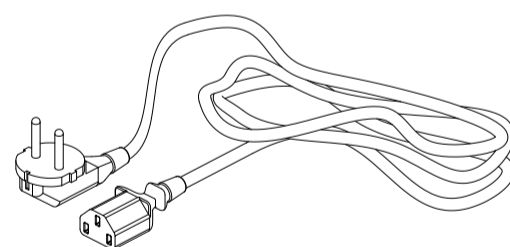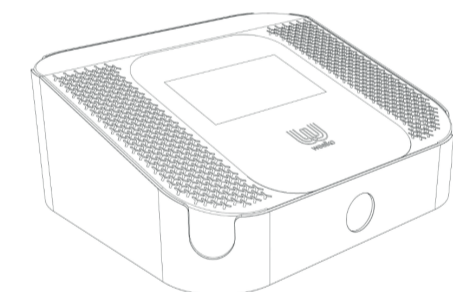

## INSTRUCTIONS OF USE

1. Connect the power cord via the rear panel.
2. Connect the accessories and negative plate properly to the rear panel.
3. Turn on the power button on the front panel and click on Weelko logo to select the desired menus.
4. Click on "mono.face" button if you want to use the face or eye electrodes or on "mono.body" if you want to use the body electrodes. Eye and face electrodes use the same connection, so in order to use one of them, the other one must be unplugged.

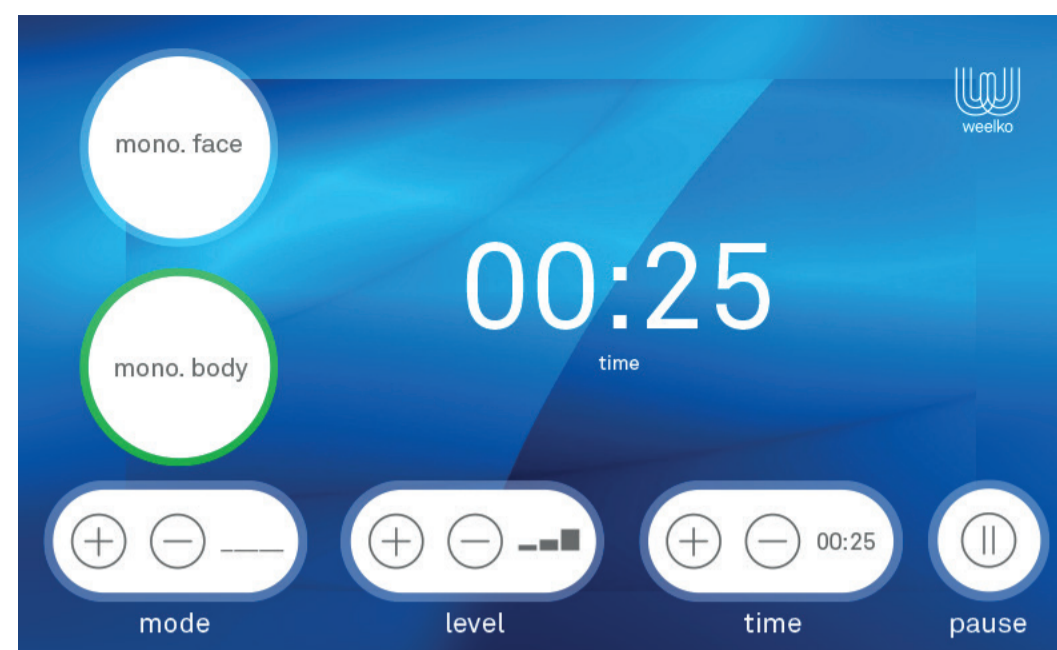

5. Apply enough glycerine or gel on the area to be treated before applying the electrodes on patient's skin.

6. The "LEVEL" menu allows adjusting 10 intensity levelsselect the other programs depending on patient's needs.

7.The "TIME" menu allows adjusting the treatment time. The default duration is 30 minutes.

8.The "MODE" menu allows choosing between 3 types of wave.

9.Press "PLAY/PAUSE" to begin or to pause the treatment.

## MAINTENANCE

- After use, clean the electrodes with a wet cloth

## CAUTIONS

• Radiofrequency treatments must not extend over a long period of time. The recommended duration is 10 minutes for facial treatments and 20 minutes for body treatments. In any case, treatments do not extend beyond 60 minutes.

• To avoid burning to the customer, never forget to put this plate in contact with the skin.

• Apply the electrodes on the customer's skin making constantly circles, without stopping of making movements. Not keep the electrode without moving at the same zone during a long period of time, the customer could be burned.

• During the treatment, check with the patient if the intensity is appropriate.

• The patient and the professional must not wear any metallic objects during the treatment.

• The professional is advised to use insulated gloves to protect hands during the treatment.

## ACCESSORIES

No.	PRODUCT
1	BODY ELECTRODES
2	FACE ELECTRODES
3	EYE ELECTRODES
4	NEGATIVE PLATE
5	MAIN UNIT
6	POWER CORD

## TECHNICAL SHEET

Weights and sizes	Packing size (cm)	51x45x22
	Gross weight (kg)	9
	Product size (cm)	34x38x15
Electrical characteristics	Rated voltage	220V ~ 240V
	Frequency	50Hz/60Hz
	Rated power	150 W